





WEB™ Intrasaccular Flow Disruptor
Revolutionizing Aneurysm Treatment

WEB System Specifications


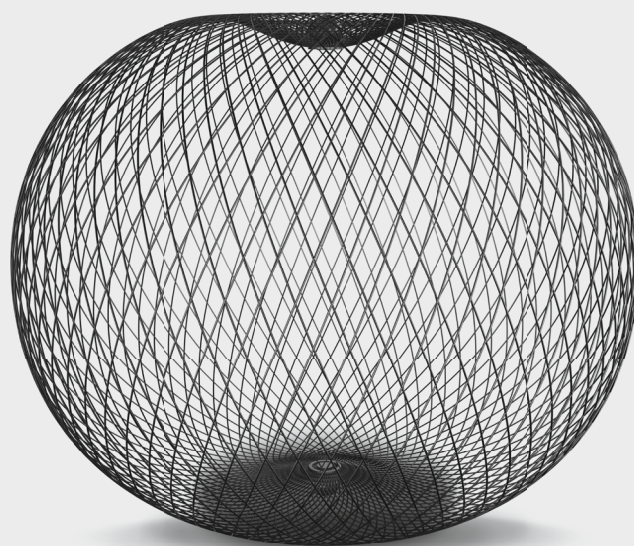


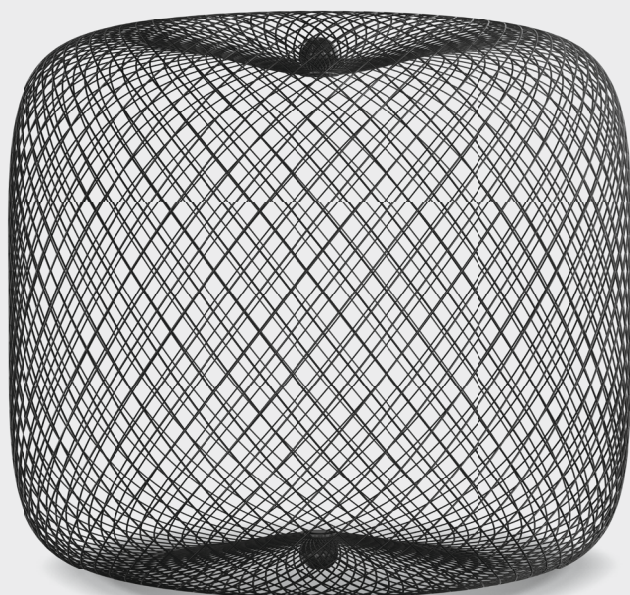

WEB SL

WEB SL Height (mm)	9								SL 11×9
	8							SL 10×8	SL 11×8
	7						SL 9×7	SL 10×7	SL 11×7
	6			SL 7×6	SL 8×6	SL 9×6	SL 10×6	SL 11×6	
	5		SL 6×5	SL 7×5	SL 8×5	SL 9×5	SL 10×5		
	4	SL 5×4	SL 6×4	SL 7×4	SL 8×4	SL 9×4			
	3	SL 4×3	SL 5×3	SL 6×3	SL 7×3	SL 8×3			
		4	5	6	7	8	9	10	11

WEB SL Diameter (mm)

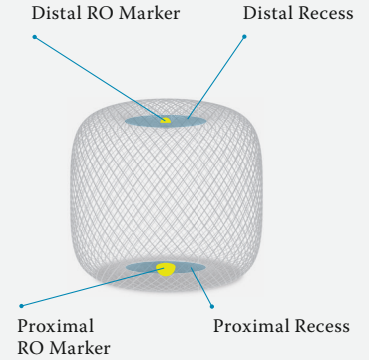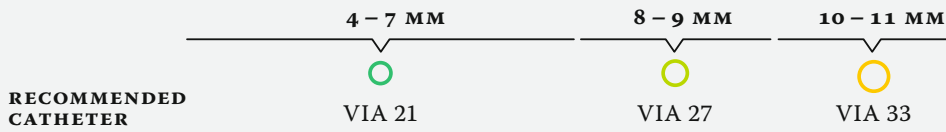

Name	Ref No.	Diameter (mm)	Height (mm)	Min. Catheter ID	Recommended Catheter
WEB 4×3	W4-4-3	4	3	.021"	VIA 21
WEB 5×3	W4-5-3	5	3	.021"	VIA 21
WEB 5×4	W4-5-4	5	4	.021"	VIA 21
WEB 6×3	W4-6-3	6	3	.021"	VIA 21
WEB 6×4	W4-6-4	6	4	.021"	VIA 21
WEB 6×5	W4-6-5	6	5	.021"	VIA 21
WEB 7×3	W4-7-3	7	3	.021"	VIA 21
WEB 7×4	W4-7-4	7	4	.021"	VIA 21
WEB 7×5	W4-7-5	7	5	.021"	VIA 21
WEB 7×6	W4-7-6	7	6	.021"	VIA 21
WEB 8×3	W2-8-3	8	3	.027"	VIA 27
WEB 8×4	W2-8-4	8	4	.027"	VIA 27
WEB 8×5	W2-8-5	8	5	.027"	VIA 27
WEB 8×6	W2-8-6	8	6	.027"	VIA 27
WEB 9×4	W2-9-4	9	4	.027"	VIA 27
WEB 9×5	W2-9-5	9	5	.027"	VIA 27
WEB 9×6	W2-9-6	9	6	.027"	VIA 27
WEB 9×7	W2-9-7	9	7	.027"	VIA 27
WEB 10×5	W2-10-5	10	5	.033"	VIA 33
WEB 10×6	W2-10-6	10	6	.033"	VIA 33
WEB 10×7	W2-10-7	10	7	.033"	VIA 33
WEB 10×8	W2-10-8	10	8	.033"	VIA 33
WEB 11×6	W2-11-6	11	6	.033"	VIA 33
WEB 11×7	W2-11-7	11	7	.033"	VIA 33
WEB 11×8	W2-11-8	11	8	.033"	VIA 33
WEB 11×9	W2-11-9	11	9	.033"	VIA 33

WEB SLS

WEB SLS Height (mm)	9.6								SLS 11
	8.6							SLS 10	
	7.6					SLS 9			
	6.6				SLS 8				
	5.6			SLS 7					
	4.6		SLS 6						
	3.6		SLS 5						
	2.6	SLS 4							
		4	5	6	7	8	9	10	11

WEB SLS Diameter (mm)

4 – 7 MM

8 – 9 MM

10 – 11 MM




RECOMMENDED CATHETER

VIA 21

VIA 27

VIA 33

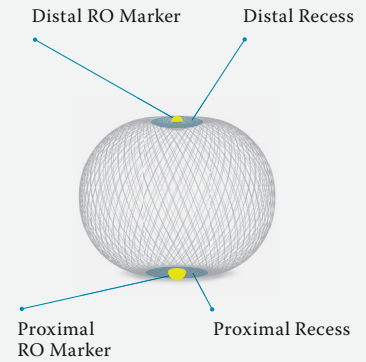


Name	Ref No.	Diameter (mm)	Min. Catheter ID	Recommended Catheter
WEB 4	W4-4-S	4	.021"	VIA 21
WEB 5	W4-5-S	5	.021"	VIA 21
WEB 6	W4-6-S	6	.021"	VIA 21
WEB 7	W4-7-S	7	.021"	VIA 21
WEB 8	W2-8-S	8	.027"	VIA 27
WEB 9	W2-9-S	9	.027"	VIA 27
WEB 10	W2-10-S	10	.033"	VIA 33
WEB 11	W2-11-S	11	.033"	VIA 33

WDC


WEB Detachment Controller

Name	Ref No.	Remarks
WDC	WDC-1	Free of Charge

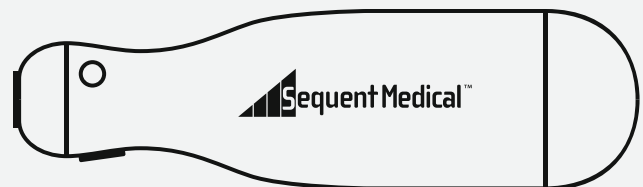


Device Selection Tables


WEB SL Device Selection Table
Treat Aneurysms Between 3 mm and 10 mm

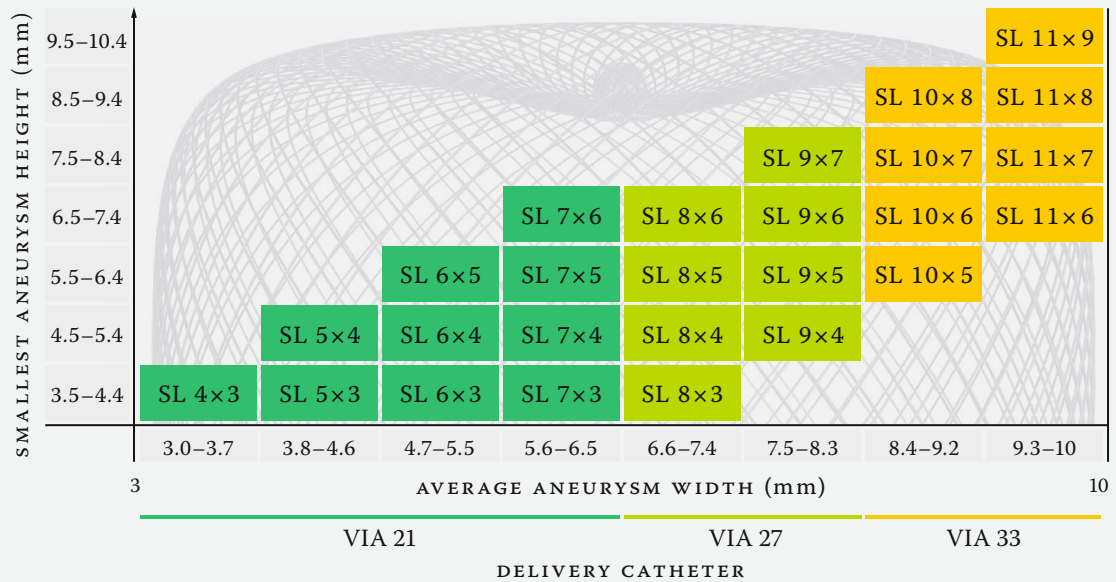

WEB SLS Device Selection Table
Treat Aneurysms Between 3 mm and 10 mm

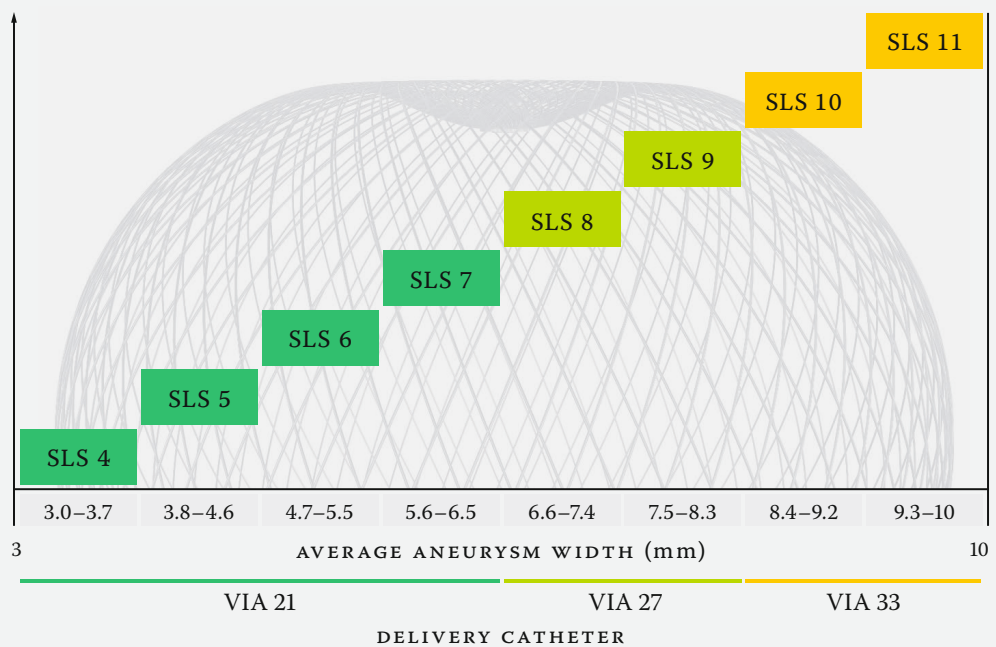


VIA Microcatheters

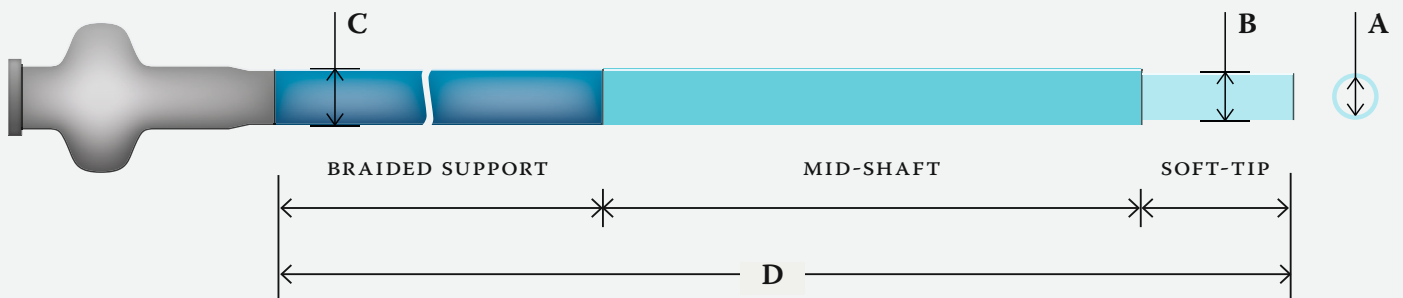

Name	Ref No.	Inner Diameter (A)	Distal Outer Diameter (B)	Proximal Outer Diameter (C)	Working Length (D)
VIA 21	VIA-21-154-01	1.6 Fr	2.5 Fr	2.8 Fr	154 cm
		0.021 in	0.033 in	0.036 in	
		0.53 mm	0.84 mm	0.91 mm	
VIA 27	VIA-27-154-01	2.1 Fr	3.0 Fr	3.2 Fr	154 cm
		0.027 in	0.039 in	0.042 in	
		0.69 mm	0.99 mm	1.07 mm	
VIA 33	VIA-33-133-01	2.5 Fr	3.4 Fr	3.8 Fr	133 cm
		0.033 in	0.045 in	0.050 in	
		0.84 mm	1.14 mm	1.27 mm	

Stable Distal Access Technique

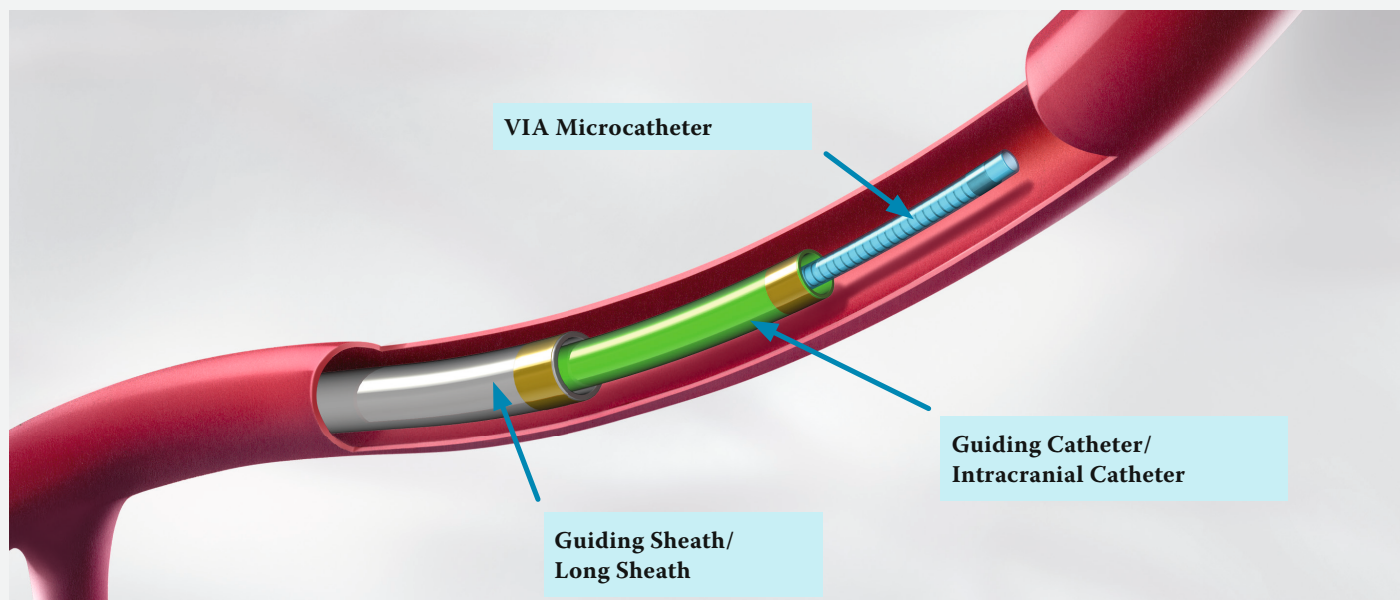

WEB SL / SLS WEB Diameter (mm)	VIA Microcatheter (Delivery Catheter)	Guiding Catheter / Intracranial Catheter	Guiding Sheath / Long Sheath
4 – 7	VIA 21 ID: 0.021" Distal OD: 2.5F/0.033" Proximal OD: 2.8F/0.036" Length: 154 cm	5F, 0.056" ID or larger, 90 – 125 cm long	6F: 80 / 90 cm long
8 – 9	VIA 27 ID: 0.027" Distal OD: 3.0F/0.039" Proximal OD: 3.2 F/0.042" Length: 154 cm	6F, 0.070" ID or larger, 90 – 125 cm long	6F: 80 / 90 cm long
10 – 11	VIA 33 ID: 0.033" Distal OD: 3.4F/0.045" Proximal OD: 3.8F/0.050" Length: 133 cm	6F, 0.070" ID or larger, 90 – 115 cm long	6F: 80 / 90 cm long



Global Headquarters / Manufacturer

Sequent Medical Inc.,
11 Columbia, Aliso Viejo, CA 92656 | USA
OFFICE +1-949 830 9600

European Headquarters

Sequent Medical GmbH
Uwierstr. 83, 53173 Bonn | Germany
OFFICE +49-228 550 791-0

Notified Body

DQS Medizinprodukte GmbH
August-Schanz-Straße 21, 60433 Frankfurt am Main | Germany
OFFICE +49-69 954 27-300

Authorized European Representative

MediMark® Europe SARL
11 rue Emile Zola – BP 2332, 38033 Grenoble Cedex 2 | France
OFFICE +33-4 7686-4322

www.sequentmedical.com



The WEB Aneurysm Embolization System and VIA Microcatheter have both received the CE mark. The WEB Aneurysm Embolization System is not approved or available for sale or use in the United States.

The WEB Aneurysm Embolization System is a class III device intended for the endovascular embolization of ruptured and unruptured intracranial aneurysms.

For complete indications, potential complications, warnings and instructions, see instructions for use (IFU provided in the device).

The device should only be used by physicians who have undergone training in all aspects of the WEB Aneurysm Embolization System procedures as prescribed by Sequent Medical Inc.

The WEB device is not currently listed in the LPPR (List des Produits et Prestations Remboursables).